



Thermal Imager
Mini2 V2/Mini2Plus V2/MiniE
User Manual



Contact Us

CONTENTS

1	Introduction	1
1.1	Thermal Imager and HIKMICRO Viewer	1
1.2	Download HIKMICRO Viewer.....	1
1.3	Connect Thermal Imager and HIKMICRO Viewer	2
1.4	User Manual	2
2	Live View.....	3
2.1	Live View	3
2.1.1	Live View Interface	3
2.1.2	Adjust Image Display	4
2.1.3	Thermal Image Calibration	7
2.1.4	Select Palettes	7
2.1.5	Adjust Display Temperature Range	8
2.1.6	Set Image Parameters.....	8
3	Temperature Measurement.....	9
3.1	Select Scene Mode.....	9
3.2	Set Temperature Measurement Parameters	11
3.3	Measure Temperature	12
3.3.1	Add Point Measurement Tool.....	12
3.3.2	Add Line Measurement Tool.....	13
3.3.3	Add Rectangle Measurement Tool.....	13
3.3.4	Set Temperature Alarm (Optional)	14
4	Capture Snapshots and Record Videos.....	15
4.1	Capture Snapshots	15
4.2	Record Videos	15
4.3	View Snapshots/Videos	15
4.4	Edit Snapshots	16
4.5	Share Snapshots and Videos	16
4.6	Generate and Share PDF Report	16
5	Update and Maintenance.....	18
5.1	Update the Imager	18
5.2	Reset the Imager	18
5.3	Error Diagnosis.....	18

1 Introduction

1.1 Thermal Imager and HIKMICRO Viewer

The thermal imager (hereinafter refers to as **the Device** or **the Imager**) is an infrared thermal camera connected to mobile devices like smartphones or pads with Android or iOS systems through Type-C and Lightning connectors.

The imager needs to work with the HIKMICRO Viewer (hereinafter refers to as **the APP**).

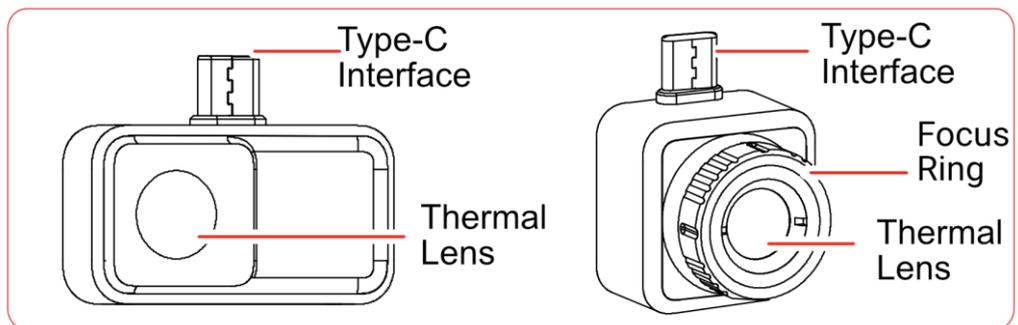


Figure 1-1 Thermal Imager Appearance



This manual describes and explains the features for multiple thermal imagers.

1.2 Download HIKMICRO Viewer

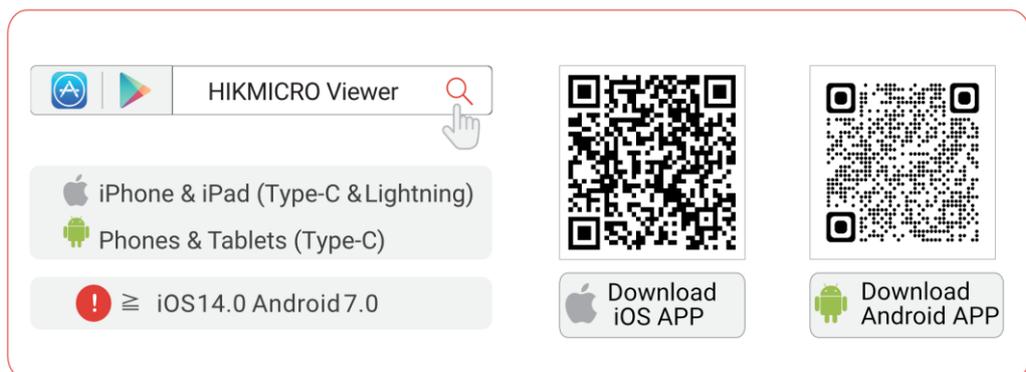


Figure 1-2 HIKMICRO Viewer QR Code

1.3 Connect Thermal Imager and HIKMICRO Viewer

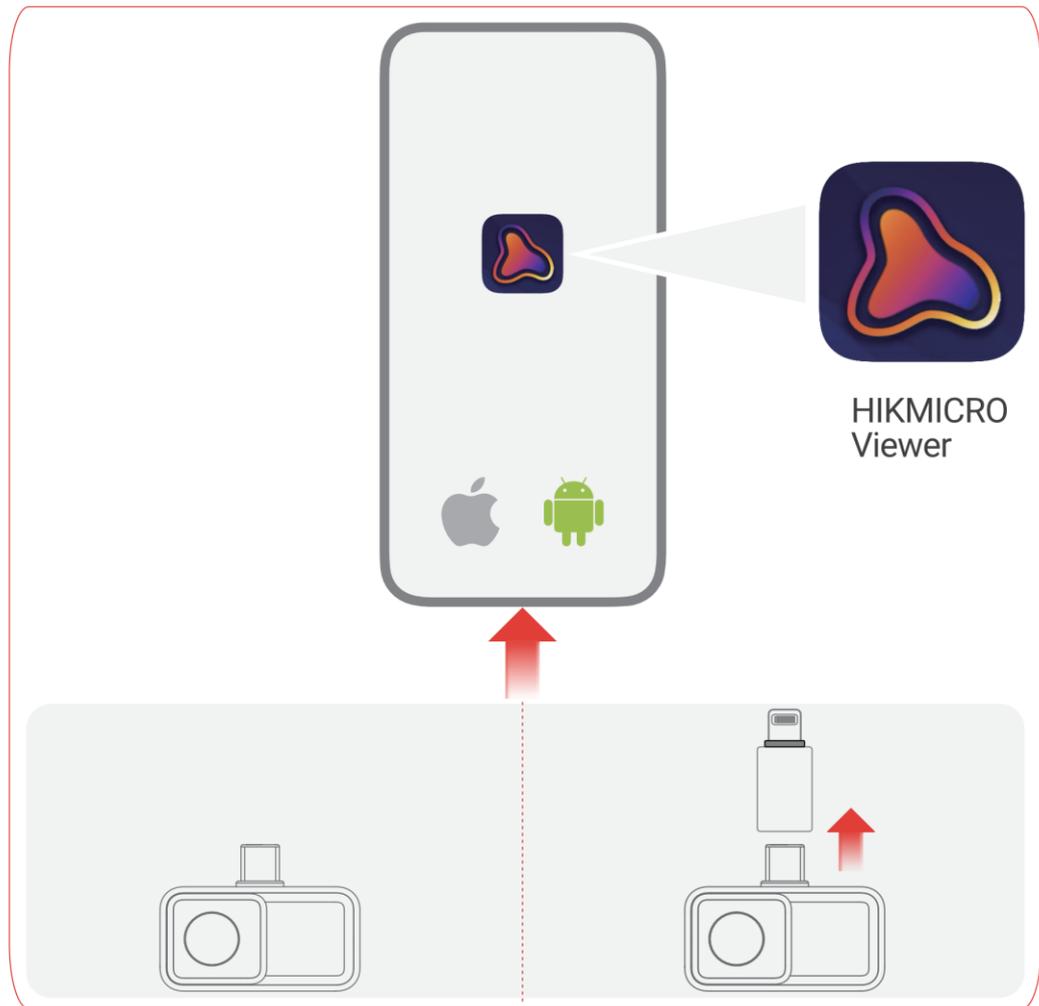


Figure 1-3 Connect Thermal Imager to the APP



- The thermal imager in figure above is for demonstration ONLY.
- If connected successfully, "Connected" will show on the home screen.
- The Lightning Adapter and the Type-C Extension Cord cannot use

together.



1.4 User Manual

In the home screen, tap **Device Info** > **Help** for detailed information about the device.

2 Live View

2.1 Live View

In **Live View**, you can adjust and calibrate thermal image, measure temperatures, change palettes, etc.

2.1.1 Live View Interface

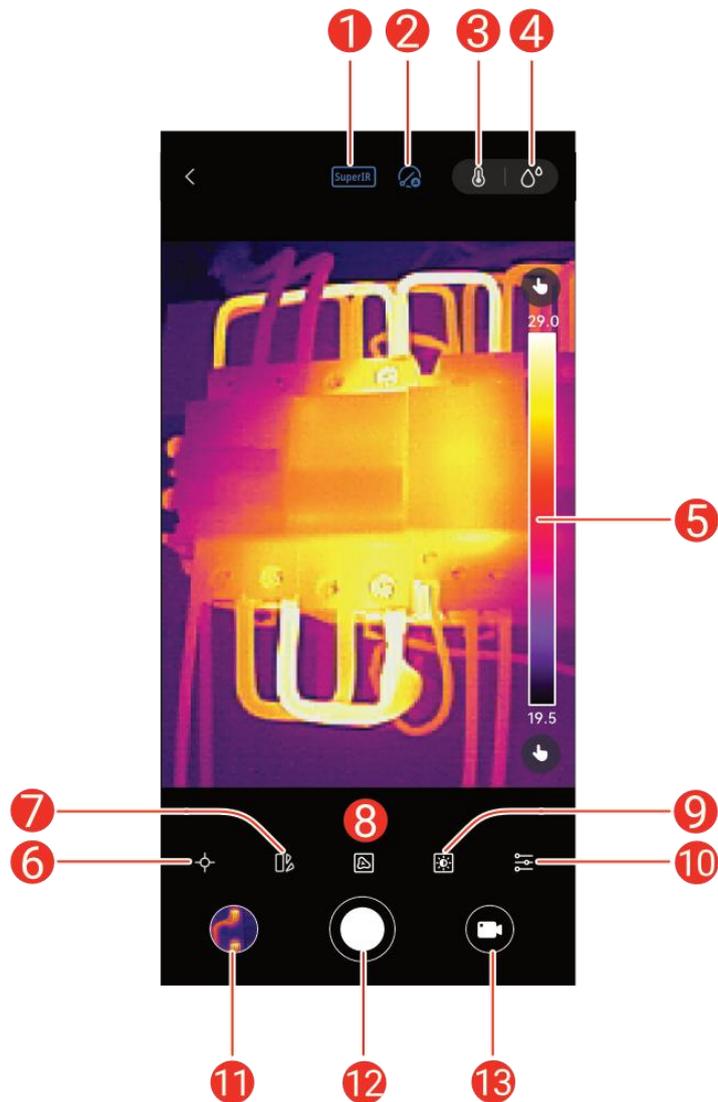


Figure 2-1 Live View Interface



This picture is for demonstration ONLY. Please refer to your actual device for available operations.

Table 2-1 Live View Interface Icons

No.	Functions	Description
1	SuperIR	Enhance the object outlines for better image display.
2	Image Calibration	Correct image uniformity to improve image quality and temperature measurement accuracy.
3	Measurement Parameters	Set key parameters such as temperature measurement distance and emissivity to ensure the measurement accuracy.
4	Scene Mode	You can switch scenes freely and perform detection quickly.
5	Temperature Scale and Display Temperature Range	Auto  : Display temperature range will be automatically adjusted Manual  : Drag the temperature value to adjust temperature range. In manual adjustment, the palette turns to focus palette mode, in which objects falling in the range remain the selected palette while the rest is displayed in white hot palette.
6	Measurement Tools	Set rules for temperature measurement.
7	Palettes	Select color styles for thermal imaging.
8	Image Mode	You can set the thermal/optical view of the device. Thermal , Visual , and Fusion are selectable.
9	Image	Adjust brightness, sharpness, contrast and color distribution.
10	Parameter	Set parameters such as temperature measurement range and temperature alarm.
11	Album	View sanpshots and videos.
12	Capture/Record	Tap to capture the image in snapshot mode or to start/stop recording in video mode.
13	Snapshot/Video Mode	Switch between snapshot and video mode.

2.1.2 Adjust Image Display

Focusing Adjustment (for Some Imagers)

Aim the thermal lens to your target, and rotate the focus ring to make the image clear.

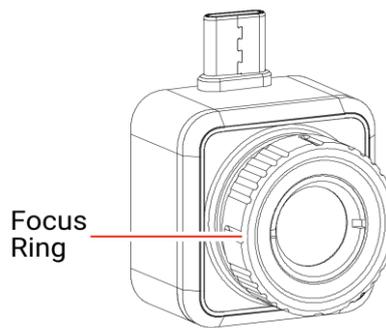


Figure 2-2 Thermal Imager with a Focus Ring



Focusing Adjustment is ONLY supported by the imager with a focus ring.

Image Rotation

Tap  >  to rotate live image by 90 degrees.

Zoom

Tap  >  to zoom in the live image. When not selected, the live image will be zoomed out.



Zoom function varies within the series. See your device for available operations.

SuperIR

Switch on  to get an enhanced thermal image. Captured thermal image with **SuperIR** is clearer than the original one.

For some series, you can select  **Performance Mode** or  **Quality Mode**.



- Compared to **Performance Mode**, **Quality Mode** provides higher image resolution but consumes more phone resource and battery power, which may reduce the live view frame rate and cause the phone to overheat.
 - If the phone performance is insufficient, it may not support **Quality Mode**. Please use the feature according to actual situation
 - **SuperIR** function varies within the series. See your device for available operations.
-

Display Mode

Tap  to select the display mode of the live view.

- : In **Thermal** mode, the device displays the thermal image.
- : In **Visual** mode, the device displays the thermal image overlaid with a visual image in the upper-left corner. You can drag the visual image frame to move it.
- : In **Fusion** mode, the device displays the thermal image of the live view outlined from visual image.



- The visual image is captured by your phone's camera. To use either **Visual** or **Fusion** mode, it is required to grant the APP permission to access your phone's camera.
- When **Fusion** is enabled, **Rotation** and **SuperIR** will be unavailable, and **Sharpness** value will reset to zero.
- **SuperIR** function is supported by some models. See your device for available operations.

Camera Alignment

To display the precise fusion view of the thermal and visual image, please follow the instructions to finish **Camera Alignment** for the first time.

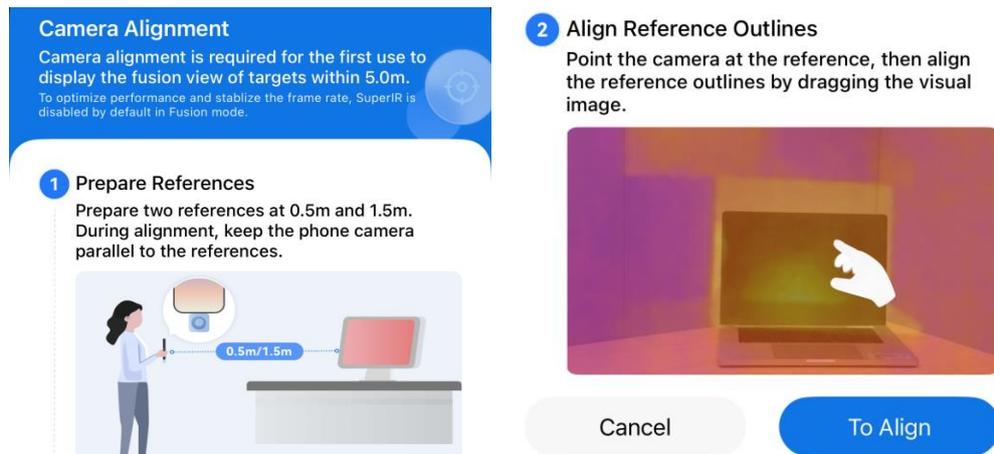


Figure 2-3 Camera Alignment

1. Prepare two references at 0.5 m and 1.5 m. During alignment, keep the phone camera parallel to the references.
2. Point the phone camera at the reference, then align the reference outlines by dragging the visual image.
3. After completing initial alignment, tap  to adjust the fusion distance based on target range. For closer targets, slide the bar to the left; for distant targets, slide it to the right until the visual and thermal image outlines are perfectly aligned.
4. If the outlines are misaligned, tap  to perform **Camera Alignment** again.



After **Camera Alignment**, partial visual light loss around the edges may occur due to differences in position and field of view (FOV) between the phone camera and the thermal imager camera. This is a normal phenomenon.

2.1.3 Thermal Image Calibration

For temperature measurement accuracy and image effect, it is recommended to conduct image calibration. It is common to have brief image freeze during image calibration.

Auto Calibration

In this mode, the imager automatically calibrates images according to its internal rules.

Tap  to enable **Auto Calibration**.

Manual Calibration

Tap  to calibrate the image for one time.

Turn off Calibration

Tap  to turn off the calibration function.



It is recommended to enable **Auto Calibration**. Otherwise, you need conduct **Manual Calibration** from time to time for the accuracy of thermal imaging and temperature measurement.

2.1.4 Select Palettes

Palettes highlights the imaging details as the image displays different colors according to temperature range.

Tap  to select appropriate palettes.

Custom Palettes and predefined palettes are available.

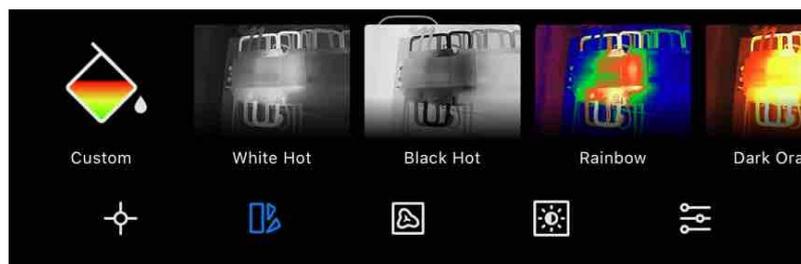


Figure 2-4 Different Palettes



- NO MORE THAN 4 colors are supported to set in the **Custom Palettes**.
 - Tap **Custom Palettes** > ⊕ to add appropriate colors. Swipe the palettes points to adjust the color distribution of the palettes bar.
 - **Custom Palettes** function is supported by some models. See your device for available operations.
-



Figure 2-5 Custom Palettes

2.1.5 Adjust Display Temperature Range

After selecting appropriate palettes, it is advisable to adjust display temperature range to highlight the thermal image of the target of interest.

Auto Adjustment

Tap , the imager will shift to **Auto Adjustment**, and the display temperature range will be automatically adjusted.

Manual Adjustment

Tap , the imager will shift to **Manual Adjustment**. It is a focus palette that you can swipe the temperature value up and down to adjust the range, focusing on the target in the set range.



Tap  >  to display or hide the temperature scale. The function varies within the series. See your actual device for available operations.

2.1.6 Set Image Parameters

For better image analysis, it is recommended to tap  to set appropriate parameters:



Brightness



Contrast



Sharpness



Color Distribution



Color Distribution supports Linear and Histogram:

- **Linear:** The mode displays relatively huge temperature gap.
 - **Histogram:** The mode displays relatively small temperature gap.
-

3 Temperature Measurement

3.1 Select Scene Mode



Scene Mode is supported by some models. See your device for available operations.

To conduct fast anomaly detection, several preset templates are included in scene mode for various detection scenarios. Users can choose an appropriate scene or customize a scene as per targets, and set temperature alarms or anomalies recognition as needed.

1. Tap  to select the scene mode, and tap **Confirm** to perform detection. The icon varies according to different scene modes.
2. Tap **Modify Parameters** to edit the default parameters such as emissivity and alarm mode, refer to the following chapters for details. Tap  to restore the default configuration of the current scene mode.

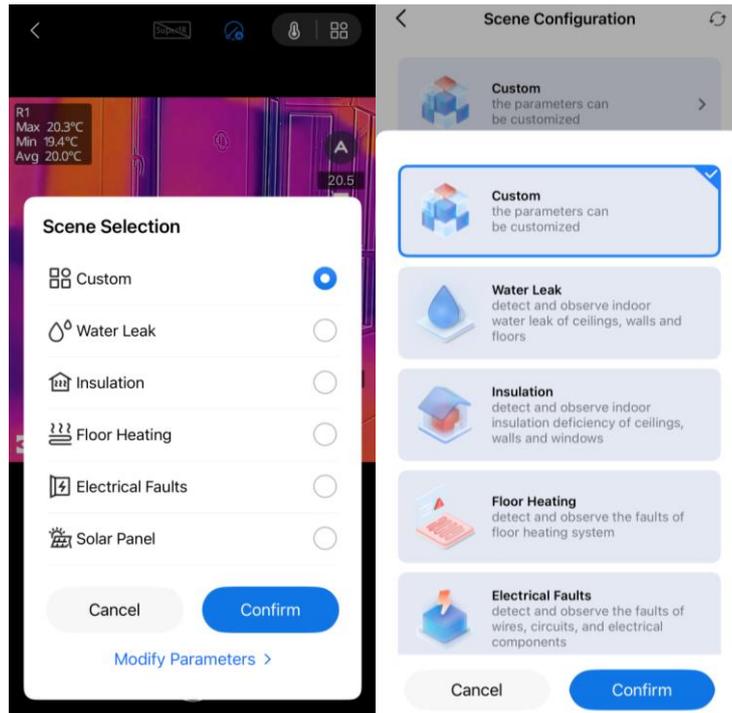


Figure 3-1 Scene Mode

- In **Custom**, **Floor Heating**, **Electrical Faults**, and **Solar Panel** mode, you can configure temperature measurement and alarm parameters.
 - **Custom**: Users can customize a mode to save desired temperature measurement parameters for future use.
 - **Floor Heating**: To detect and observe the faults of floor heating system.
 - **Electrical Faults**: To detect and observe the faults of wires, circuits, electrical components, terminators, etc.
 - **Solar Panel**: To detect and observe the faults of solar panels.
- In **Water Leak** and **Insulation** mode, you can configure **SuperScene**. The feature can assist in fast recognition of the location of water leak points and defective heat-insulated areas.



Temperature Range and **Temperature Alarm** settings are not supported in **Water Leak** and **Insulation** mode.

- **Water Leak**: To inspect the water leak of building ceilings, walls and floors indoors. When **SuperScene** is enabled and water leak anomalies are detected, the suspect point will be marked in the live view.



Figure 3-2 Water Leak Anomalies Recognition

- Insulation: To detect indoor insulation deficiency of building walls, ceilings. When **SuperScene** is enabled and insulation anomalies are detected, the suspect point will be marked in the live view.



Figure 3-3 Insulation Anomalies Recognition



- Due to the complexity of onsite scenarios, **SuperScene** cannot achieve 100% accuracy. For example, missed or even wrong reporting emerges when temperature difference of the areas with leak anomalies is too subtle to be recognized, etc. It is recommended to give a second diagnosis based on **SuperScene** results.
 - The algorithm of **SuperScene** is being updated, please update the device firmware and APP software version promptly for optimal performance.
-

3.2 Set Temperature Measurement Parameters

For more accurate measurement, tap  to set parameters before temperature measurement.

1. Tap  to set thermometry distance and emissivity.
 - Distance: Set the distance between the target and the imager.
 - Emissivity: Select or customize the emissivity of the target.
2. Tap  >  to set the temperature measurement range.

In the home screen, tap **Settings > General > Unit Settings**. You can set temperature unit and distance unit as needed.



You can tap  to select scene mode and directly use the recommended emissivity and distance preset for each scene. Temperature range settings are not supported in **Water Leak** and **Insulation** scene mode.

3.3 Measure Temperature

Measure temperature with tools. Available tools are **Point**, **Line** and **Rectangle**.

3.3.1 Add Point Measurement Tool

1. Tap  to add point tools.

Table 3-1 Point Measurement Tools

Icon	Function	Description
	Center Point	Display the real-time temperature of the center of the live image.
	Hot Point	Display the real-time highest temperature in the Live View .
	Cold Point	Display the real-time lowest temperature in the Live View .
	Custom Point	Display the temperature of a user-defined point.



Tap  to clear all measurement tools.

2. **Optional:** Edit the point

Move Point: Drag or tap the point to desired locations.

Remove Point:

- Tap  again to turn off the custom mode
- Tap the point
- Tap the pop-up  button



NO MORE THAN 3 custom points are supported to set on the Live View.

3.3.2 Add Line Measurement Tool



Line Measurement Tool is supported by some models. See your device for available operations.

1. Tap  >  to add a line on the **Live View**

2. **Optional:** Edit the line

Move Line: Drag the line to move it

Resize Line: spread fingers apart and pinch them together to adjust its size.

Remove Line:

- Tap the line
- Tap  on the pop-up window to remove it

3. **Optional:** Show/Hide Temperature Result

- Tap the line
- Tap  to show/hide the highest/lowest/average temperature
- Tap **OK** to confirm the settings

3.3.3 Add Rectangle Measurement Tool

1. Tap  >  to add a rectangle on the **Live View**.

2. **Optional:** Edit the rectangle.

Move Rectangle:

- Drag the rectangle
- Tap any part outside of the rectangle to end the moving process

Resize Rectangle:

- Tap  to turn off the rectangle tool
- Tap the rectangle and drag its vertex
- Tap any part outside of the rectangle to end the resizing process

Remove Rectangle:

- Tap the rectangle, and it will pop up an edition window
- Tap  to remove it

3. **Optional:** Show/Hide Temperature Result

- Tap the rectangle, and it will pop up an edition window.
- Tap  to show/hide the highest/lowest/average temperature
- Tap **OK** to confirm the settings



NO MORE THAN 3 rectangles are supported to set on the Live View.

3.3.4 Set Temperature Alarm (Optional)

The exceptional temperature will cause the flashing **High Temp** or **Low Temp** at the bottom of the **Live View** and the vibration.

1. Tap .
2. Tap  to input the maximum value of **High Temp** and the minimum value of **Low Temp** in the pop-up window.



Threshold range of temperature exception alarm is -20°C ~ 400°C.

3. Slide  to switch on the **High Temp** alarm or the **Low Temp** Alarm respectively.



It does NOT support to enable **High Temp** alarm and **Low Temp** alarm at the same time.

4. Tap **OK** to confirm the settings.



You can tap  to select the scene mode to perform quick detection with preset parameter templates, or customize the temperature alarm parameters for different scenes. Temperature alarm settings are not supported in **Water Leak** and **Insulation** scene mode.

4 Capture Snapshots and Record Videos

4.1 Capture Snapshots

If you need to save snapshots to your phone, please tap **Settings > General > Save Pictures and Videos to Phone**.

Tap  to capture thermal images and save them to the APP album and your phone.

4.2 Record Videos

1. Tap  to shift into **Video** mode.

2. Tap  to start the video recording, and tap again to stop.



Snapshot and **Video** modes can be freely switched around.

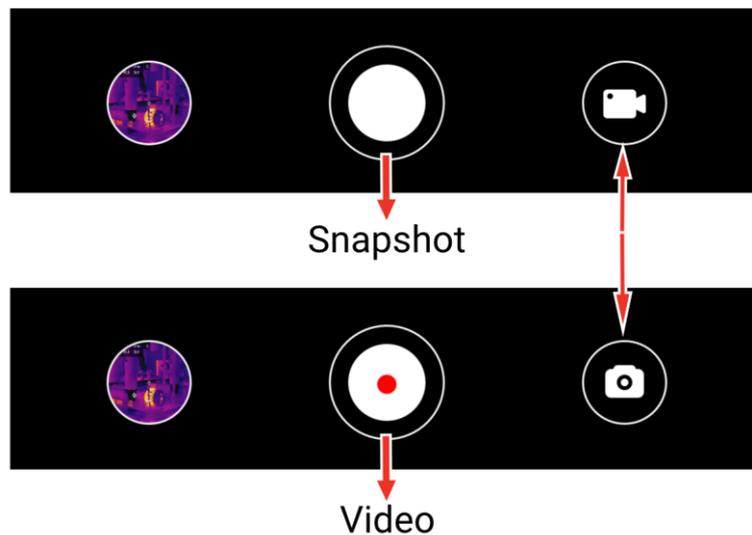


Figure 4-1 Switch Between Snapshot and Video Modes

4.3 View Snapshots/Videos

You can view the pictures and videos saved in the album as follows:

- Tap the snapshot or video on the lower left corner on the **Live View**.

- Tap the snapshot or video on the lower left corner on the **Live View**, then tap , and you can view all the snapshots and videos.
- Tap  in the home scree, and you can view all the snapshots and videos

4.4 Edit Snapshots

You can adjust the parameters of the snapshot to get more accurate temperature results.

1. Enter to the **Album** and select the snapshot.
2. Tap  to enable editing functions.

Table 4-1 Icons for Snapshots Editing

Icon	Function	Description
	Measurement	Adjust the temperature values on the rectangular box on the Live View . Tap again to hide the results.
	Image Mode	Select image modes, including Thermal, Visual, and Fusion .
	Level and Span	Select Auto, Manual and 1-Tap modes to highlight certain temperature range.
	Palettes	Select palettes.
	Color Alarms	Set the highest and lowest temperature or certain temperature range of the snapshot to highlight the required areas.
	Parameter	Adjust emissivity, distance, and environment temperature. You can also remark on the picture.



- **Video** does NOT support editing functions.
- The temperature range of **Color Alarms** is $-20^{\circ}\text{C} \sim 150^{\circ}\text{C}$.

4.5 Share Snapshots and Videos

1. Enter to **Albums**, and tap  to select the snapshots and videos.
2. Tap  to share the snapshots and videos with the third party.
3. **Optional:** Tap  to save snapshots and videos to your phone.

4.6 Generate and Share PDF Report

1. Enter to the **Album** and select the snapshot.
2. Tap  to edit the report information.



File Name is a MUST.

3. Tap **Next** > ✓ to generate a PDF report.
 4. Tap  to share the report with the third party.
-



Video does NOT support PDF report generation and sharing.

5 Update and Maintenance

5.1 Update the Imager

For better operation experience, it is recommended to update to the latest version in time. The imager update is as follows:

- In the home screen, tap **Device Upgrade > Check for Updates**.
- In the home screen, tap **Device Info > Device Upgrade > Check for Updates**.

5.2 Reset the Imager

Tap **Device Info > Reset > OK** to restore the thermal imager.



Be careful to use this function, or the data will be lost.

5.3 Error Diagnosis

If you encounter some device exception during the operation, error diagnosis can help you quickly troubleshoot. Feedback paths are as follows:

- In the home screen, tap **Device Info > Device Diagnosis**.
- In the home screen, tap **Settings > Support** to get online service support, hotline support or to submit logs.

Legal Information

©Hangzhou Microimage Software Co., Ltd. All rights reserved.

About this Manual

The Manual includes instructions for using and managing the Product. Pictures, charts, images and all other information hereinafter are for description and explanation only. The information contained in the Manual is subject to change, without notice, due to firmware updates or other reasons. Please find the latest version of this Manual at the HIKMICRO website (www.hikmicrotech.com/).

Please use this Manual with the guidance and assistance of professionals trained in supporting the Product.

Trademarks Acknowledgement

 **HIKMICRO** and other HIKMICRO's trademarks and logos are the properties of HIKMICRO in various jurisdictions.

Other trademarks and logos mentioned are the properties of their respective owners.

LEGAL DISCLAIMER

TO THE MAXIMUM EXTENT PERMITTED BY APPLICABLE LAW, THIS MANUAL AND THE PRODUCT DESCRIBED, WITH ITS HARDWARE, SOFTWARE AND FIRMWARE, ARE PROVIDED "AS IS" AND "WITH ALL FAULTS AND ERRORS". HIKMICRO MAKES NO WARRANTIES, EXPRESS OR IMPLIED, INCLUDING WITHOUT LIMITATION, MERCHANTABILITY, SATISFACTORY QUALITY, OR FITNESS FOR A PARTICULAR PURPOSE. THE USE OF THE PRODUCT BY YOU IS AT YOUR OWN RISK. IN NO EVENT WILL HIKMICRO BE LIABLE TO YOU FOR ANY SPECIAL, CONSEQUENTIAL, INCIDENTAL, OR INDIRECT DAMAGES, INCLUDING, AMONG OTHERS, DAMAGES FOR LOSS OF BUSINESS PROFITS, BUSINESS INTERRUPTION, OR LOSS OF DATA, CORRUPTION OF SYSTEMS, OR LOSS OF DOCUMENTATION, WHETHER BASED ON BREACH OF CONTRACT, TORT (INCLUDING NEGLIGENCE), PRODUCT LIABILITY, OR OTHERWISE, IN CONNECTION WITH THE USE OF THE PRODUCT, EVEN IF HIKMICRO HAS BEEN ADVISED OF THE POSSIBILITY OF SUCH DAMAGES OR LOSS.

YOU ACKNOWLEDGE THAT THE NATURE OF THE INTERNET PROVIDES FOR INHERENT SECURITY RISKS, AND HIKMICRO SHALL NOT TAKE ANY

RESPONSIBILITIES FOR ABNORMAL OPERATION, PRIVACY LEAKAGE OR OTHER DAMAGES RESULTING FROM CYBER-ATTACK, HACKER ATTACK, VIRUS INFECTION, OR OTHER INTERNET SECURITY RISKS; HOWEVER, HIKMICRO WILL PROVIDE TIMELY TECHNICAL SUPPORT IF REQUIRED.

YOU AGREE TO USE THIS PRODUCT IN COMPLIANCE WITH ALL APPLICABLE LAWS, AND YOU ARE SOLELY RESPONSIBLE FOR ENSURING THAT YOUR USE CONFORMS TO THE APPLICABLE LAW. ESPECIALLY, YOU ARE RESPONSIBLE, FOR USING THIS PRODUCT IN A MANNER THAT DOES NOT INFRINGE ON THE RIGHTS OF THIRD PARTIES, INCLUDING WITHOUT LIMITATION, RIGHTS OF PUBLICITY, INTELLECTUAL PROPERTY RIGHTS, OR DATA PROTECTION AND OTHER PRIVACY RIGHTS. YOU SHALL NOT USE THIS PRODUCT FOR ILLEGAL HUNTING ANIMALS, INVASION OF PRIVACY OR ANY OTHER PURPOSE WHICH IS ILLEGAL OR DETRIMENTAL TO THE PUBLIC INTEREST. YOU SHALL NOT USE THIS PRODUCT FOR ANY PROHIBITED END-USES, INCLUDING THE DEVELOPMENT OR PRODUCTION OF WEAPONS OF MASS DESTRUCTION, THE DEVELOPMENT OR PRODUCTION OF CHEMICAL OR BIOLOGICAL WEAPONS, ANY ACTIVITIES IN THE CONTEXT RELATED TO ANY NUCLEAR EXPLOSIVE OR UNSAFE NUCLEAR FUEL-CYCLE, OR IN SUPPORT OF HUMAN RIGHTS ABUSES.

IN THE EVENT OF ANY CONFLICTS BETWEEN THIS MANUAL AND THE APPLICABLE LAW, THE LATTER PREVAILS.

Regulatory Information

These clauses apply only to the products bearing the corresponding mark or information.

EU Conformity Statement



This product and - if applicable - the supplied accessories too are marked with "CE" and comply therefore with the applicable harmonized European standards listed under the Directive 2014/30/EU (EMCD), Directive 2014/35/EU (LVD), Directive 2011/65/EU (RoHS).



Directive 2012/19/EU (WEEE Directive): Products marked with this symbol cannot be disposed of as unsorted municipal waste in the European Union. For proper recycling, return this product to your local supplier upon the purchase of equivalent new equipment, or dispose of it at designated collection points. For more information see: www.recyclethis.info

According to the Waste Electrical and Electronic Equipment Regulations 2013: Products marked with this symbol cannot be disposed of as unsorted municipal waste in the United Kingdom. For proper recycling, return this product to your local supplier upon the purchase of equivalent new equipment, or dispose of it at designated collection points. For more information see: www.recyclethis.info.

Industry Canada ICES-003 Compliance

This device meets the CAN ICES- 003 (B) / NMB- 003 (B) standards requirements.

INFORMATIONEN FÜR PRIVATE HAUSHALTE

1. Getrennte Erfassung von Altgeräten:

Elektro- und Elektronikgeräte, die zu Abfall geworden sind, werden als Altgeräte bezeichnet. Besitzer von Altgeräten haben diese einer vom unsortierten Siedlungsabfall getrennten Erfassung zuzuführen. Altgeräte gehören insbesondere nicht in den Hausmüll, sondern in spezielle Sammel- und Rückgabesysteme.

2. Batterien und Akkus sowie Lampen:

Besitzer von Altgeräten haben Altbatterien und Altakkumulatoren, die nicht vom Altgerät umschlossen sind, die zerstörungsfrei aus dem Altgerät entnommen werden können, im Regelfall vor der Abgabe an einer Erfassungsstelle vom Altgerät zu trennen. Dies gilt nicht, soweit Altgeräte einer Vorbereitung zur Wiederverwendung unter Beteiligung eines öffentlich-rechtlichen Entsorgungsträgers zugeführt werden.

3. Möglichkeiten der Rückgabe von Altgeräten:

Besitzer von Altgeräten aus privaten Haushalten können diese bei den Sammelstellen der öffentlich-rechtlichen Entsorgungsträger oder bei den von Herstellern oder Vertriebern im Sinne des ElektroG eingerichteten Rücknahmestellen unentgeltlich abgeben. Rücknahmepflichtig sind Geschäfte mit einer Verkaufsfläche von mindestens 400 m² für Elektro- und Elektronikgeräte sowie diejenigen Lebensmittelgeschäfte mit einer Gesamtverkaufsfläche von mindestens 800 m², die mehrmals pro Jahr oder dauerhaft Elektro- und Elektronikgeräte anbieten und auf dem Markt bereitstellen. Dies gilt auch bei Vertrieb unter Verwendung von Fernkommunikationsmitteln, wenn die Lager- und Versandflächen für Elektro- und Elektronikgeräte mindestens 400 m² betragen oder die gesamten Lager- und Versandflächen mindestens 800 m² betragen. Verreiber haben die Rücknahme grundsätzlich durch geeignete Rückgabemöglichkeiten in zumutbarer Entfernung zum jeweiligen Endnutzer zu gewährleisten. Die Möglichkeit der unentgeltlichen Rückgabe eines Altgerätes besteht bei rücknahmepflichtigen Verreibern unter anderem dann, wenn ein neues gleichartiges Gerät, das im Wesentlichen die gleichen Funktionen erfüllt, an einen Endnutzer abgegeben wird.

4. Datenschutz-Hinweis:

Altgeräte enthalten häufig sensible personenbezogene Daten. Dies gilt insbesondere für Geräte der Informations- und Telekommunikationstechnik wie Computer und Smartphones. Bitte beachten Sie in Ihrem eigenen Interesse, dass für die Löschung der Daten auf den zu entsorgenden Altgeräten jeder Endnutzer selbst verantwortlich ist.

5. Bedeutung des Symbols „durchgestrichene Mülltonne“:



Das auf Elektro- und Elektronikgeräten regelmäßig abgebildete Symbol einer durchgestrichenen Mülltonne weist darauf hin, dass das jeweilige Gerät am Ende seiner Lebensdauer getrennt vom unsortierten Siedlungsabfall zu erfassen ist.

COMPLIANCE NOTICE: The thermal series products might be subject to export controls in various countries or regions, including without limitation, the United States, European Union, United Kingdom and/or other member countries of the Wassenaar Arrangement. Please consult your professional legal or compliance expert or local government authorities for any necessary export license requirements if you intend to

Thermal Imager User Manual

transfer, export, re- export the thermal series products between different countries.

Safety Instruction

These instructions are intended to ensure that user can use the product correctly to avoid danger or property loss.

Laws and Regulations

Use of the product must be in strict compliance with the local electrical safety regulations.

Technical Support

<https://www.hikmicrotech.com/en/contact-us.html> portal will help you as a HIKMICRO customer to get the most out of your HIKMICRO products. The portal gives you access to our support team, software and documentation, service contacts, etc.

Maintenance

- DO NOT maintain the camera when it is powered on, or it may cause electric shock! If the product does not work properly, please contact your dealer or the nearest service center. We shall not assume any responsibility for problems caused by unauthorized repair or maintenance.
- Wipe the device gently with a clean cloth and a small quantity of ethanol, if necessary.
- If the equipment is used in a manner not specified by the manufacturer, the protection provided by the device may be impaired.

Using Environment

- Make sure the running environment meets the requirement of the device. The operating temperature shall be -10 °C to 50 °C (14 °F to 122 °F), and the operating humidity shall be 95% or less.
- Place the device in a dry and well-ventilated environment.
- DO NOT expose the device to high electromagnetic radiation or dusty environments.
- DO NOT aim the lens at the sun or any other bright light.
- When any laser equipment is in use, make sure that the device lens is not exposed to the laser beam, or it may burn out.
- The device is suitable for indoor use only.

Transportation

- Keep the device in original or similar packaging while transporting it.
- Keep all wrappers after unpacking them for future use. In case of any failure occurred, you need to return the device to the factory with the original wrapper. Transportation without the original wrapper may

result in damage on the device and the company shall not take any responsibilities.

- Do not drop the product or subject it to physical shock. Keep the device away from magnetic interference.

Emergency

If smoke, odor, or noise arises from the device, immediately turn off the power, unplug the power cable, and contact the service center.

Manufacture Address

Room 313, Unit B, Building 2, 399 Danfeng Road, Xixing Subdistrict,
Binjiang District, Hangzhou, Zhejiang 310052, China
Hangzhou Microimage Software Co., Ltd.



HIKMICRO

See the World in a New Way